

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#1

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008501
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	0846	34	14F23-11-5-10 C1307252	.100	20		.097			X	Lee	17046	

Prepared by:
Douglas C. Talbot
06-23-14
Expires on:
06-23-16

```

08/15/14 08:50
NS4 Serial no: 008501
Version no: 4797

No. Date Time ZDHC
Calibration 08/30/09 15:40 .100

Test Result
0001 08/05/14 02:20 .091
0002 08/05/14 02:22 .004
0003 08/06/14 00:55 .122
0004 08/06/14 00:57 .123
0005 08/08/14 00:13 .200
0006 08/08/14 00:20 .219
0007 08/11/14 20:09 .049
0008 08/13/14 01:40 .236
0009 08/13/14 01:51 .207
0010 08/13/14 01:53 .220
0011 08/15/14 08:49 .097
    
```

Push Ho. 3 to erase,
or Power down to retain

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#2

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	ID. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018785
--------------------------------	-----------------	--------------------------------------	---------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR/SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	0849	34	14F23-11-5-10 C1307252	.100	21		.100			X		Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14</p> <p>Expires on: 06-23-16</p>														
<div style="border: 1px solid black; padding: 5px; text-align: center;"> <p>08/15/14 08:52 AS4 Serial no: 010785 Version no: 4797</p> <p>No. Date Time ZBAC Calibration 07/18/08 13:27 .100</p> <p>Test Result 0001 08/07/14 07:28 .090 0002 08/07/14 07:23 .091 0003 08/15/14 08:52 .100</p> <p>Push No. 3 to erase or power down to retain</p> </div>														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#3

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008546
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	0851	34	14F23-11-5-10	.100	22		.101			X		Lee	17046	
			C1307252											
<p>Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16</p>														
<p>Test Result 08/01/14 23:00 .184 08/01/14 23:06 .155 08/01/14 23:10 .183 08/03/14 03:53 .171 08/09/14 18:44 .233 08/09/14 18:47 .214 08/15/14 08:53 .161</p> <p>No. Date Time ZWAC Calibration 06/28/13 16:36 .100</p> <p>08/15/14 09:54 NSA Serial not MRO:AC Version not 4/97</p> <p>Push No. 3 to erase or power down to retain</p>														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#4

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 082659
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	0900	34	14F23-11-5-10	.100	21		.099			X		Lee	17046	
			C1307252											

Prepared by:
Douglas C. Talbot
06-23-14
Expires on:
06-23-16

08/15/14 09:08
NS4 Serial no: 082659
Version no: 4797

No. Date Time ZBAC
Calibration
08/28/14 09:04 .100

Test Result
0801 08/18/14 15:05 .010
0802 08/15/14 09:00 .099

Push No. 5 to power
or power down to retain

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#5

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008559
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	0911	34	14F23-11-5-10 C1307252	.100	20		.103			X		Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14</p> <p>Expires on: 06-23-16</p> <p>Test Result 0001 08/15/14 09:28 .100</p> <p>Calibration 11/30/11 08:55 .100</p> <p>No. Date Time ZHMC 4797</p> <p>08/15/14 09:21 004 Serial No: 008559 Version No: 4797</p> <p>Push No. 3 LO 07:30:05</p>														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

6

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008580
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	0914	34	14F23-11-5-10 C1307252	.100	21		.100			X		Lee	17046	
Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16														
Test Result 0001 08/07/14 01:39 .152 0002 08/07/14 01:39 .147 0003 08/15/14 09:17 .100 No. Date Time %BAC Calibration 03/06/14 12:39 .100 08/15/14 09:20 AS4 Serial no: 0085800 Version no: 4797 Push No. 3 to erase or power down to retain of power down to retain														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#7

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 083032
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	0910	34	14F23-11-5-10	.100	22	.099			X		Lee	17046		
			C1307252											
<p>Prepared by: Douglas C. Talbot 06-23-14</p> <p>Expires on: 06-23-16</p>														
<p style="text-align: center;"> Test Result 0801 08/05/14 08:10 .074 0802 08/05/14 08:13 .075 0803 08/07/14 02:25 .065 0804 08/07/14 02:28 .067 0805 08/07/14 03:11 .166 0806 08/07/14 03:19 .135 0807 08/14/14 01:48 .019 0808 08/14/14 02:10 .034 0809 08/14/14 02:13 .033 0810 08/15/14 09:17 .099 </p> <p style="text-align: center;"> No. Date Time ZRAC Calibration 02/17/14 09:01 .100 </p> <p style="text-align: center;"> 08/15/14 09:17 PAS Serial no: 083032 Version no: 4797 </p> <p style="text-align: center;"> Push No. 3 to erase, or Power down to retain </p>														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG
CHP 202K (Rev. 8-08) OPI 051

#3

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008620
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	0921	34	14F23-11-5-10 C1307252	.100	21		099			X		Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14</p> <p>Expires on: 06-23-16</p>														
<p>Test Result 0001 08/05/14 00:23 .088 0002 08/05/14 00:25 .084 0003 08/05/14 02:16 .021 0004 08/05/14 02:20 .058 0005 08/08/14 02:33 .000 0006 08/08/14 04:22 .190 0007 08/08/14 04:24 .191 0008 08/15/14 09:27 .099</p> <p>No. Date Time ZMNC Calibration 01/30/13 14:34 .100</p> <p>08/15/14 09:28 HSA Serial not 008620 Version not 4797</p> <p>Push No. 3 to erase or power down to retain</p>														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#9

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 082957
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS	
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO					
08/15/2014	0927	34	14F23-11-5-10	.100	22		.100		X		Lee	17046			
			C1307252												
			Prepared by:												
			Douglas C. Talbot												
			06-23-14												
			Expires on:												
			06-23-16												
<div style="text-align: right;"> 08/15/14 09:28 VSA Serial no: 082957 Version no: 4797 No. Date Time ZHAC Calibration 02/17/14 08:52 .100 Test Result 0001 08/15/14 09:28 .100 Push No. 5 to erase, or power down to retain </div>															

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

#10

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 077505
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)		PAS	PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	ID. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)				
08/15/2014		14F23-11-5-10		.100						Lee	17046	B.D. OUT FOR SERVICE
		C1307252										
		Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16										

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#11

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 077479
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	ID NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	0929	34	14F23-11-5-10 C1307252	.100	20	098			X		Lee	17046		
Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16														
Push No. 3 to erase, or power down to retain														
Test Result 0001 08/15/14 09:30 .098														
No. Date Time %BAC Calibration 02/17/14 09:10 .100														
08/15/14 09:31 NSA Serial no: 077479 Version no: 4797														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#12

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 082660
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	0932	34	14F23-11-5-10	.100	21		.101			X		Lee	17046	
			C1307252											
Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16														

No.	Date	Time	Temp	Result
0001	08/01/14	09:23	.097	
0002	08/02/14	02:29	.000	
0003	08/02/14	02:30	.000	
0004	08/02/14	03:52	.160	
0005	08/02/14	03:54	.176	
0006	08/02/14	03:59	.000	
0007	08/03/14	02:22	.113	
0008	08/03/14	02:24	.108	
0009	08/04/14	02:31	.009	
0010	08/04/14	02:33	.009	
0011	08/10/14	02:14	.000	
0012	08/10/14	02:15	.000	
0013	08/10/14	02:57	.000	
0014	08/10/14	03:55	.055	
0015	08/10/14	03:58	.054	
0016	08/10/14	05:08	.000	
0017	08/10/14	05:10	.000	
0018	08/11/14	02:18	.201	
0019	08/11/14	02:20	.156	
0020	08/11/14	02:22	.158	
0021	08/11/14	02:24	.178	
0022	08/11/14	02:25	.192	
0023	08/15/14	09:32	.101	

Test Result

08/15/14 09:33
AS4 Serial no: 082660
Version no: 4797

No. Date Time Temp
Calibration
02/12/14 09:16 .100

Push No. 3 to erase,
or power down to retain

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#13

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008709
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	0936	34	14F23-11-5-10 C1307252	.100	21	.102			X		Lee	17046	
			Prepared by:										
			Douglas C. Talbot										
			06-23-14										
			Expires on:										
			06-23-16										

Test Result
 08/01 08/03/14 12:55 .834
 08/02 08/03/14 17:57 .822
 08/03 08/15/14 09:41 .102
 Calibration
 02/17/14 09:27 .100
 No. Date Time ZMAC
 08/15/14 09:41
 AS4 Serial no: 008709
 Version no: 4797
 08/15/14 09:41
 Push No. 3 to erase,
 or lower down to retain

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#14

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008714
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	ID. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	09:39	34	14F23-11-5-10 C1307252	.100	21	104			X			Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14</p> <p>Expires on: 06-23-16</p>														
<p>Test Result</p> <p>08/15/14 09:46 AS4 Serial no: 0808/14 Version no: 4797</p> <p>No. Date Time ZBAC Calibration 08/11/04 14:05 .100</p> <p>Test Result 0001 08/01/14 22:08 .071 0002 08/01/14 22:10 .078 0003 08/01/14 22:12 .072 0004 08/02/14 02:51 .172 0005 08/02/14 02:54 .178 0006 08/02/14 02:57 .199 0007 08/03/14 02:39 .201 0008 08/03/14 04:08 .201 0009 08/03/14 04:11 .204 0010 08/10/14 03:10 .214 0011 08/10/14 03:15 .225 0012 08/10/14 03:29 .128 0013 08/10/14 04:32 .121 0014 08/10/14 20:52 .286 0015 08/10/14 20:56 .228 0016 08/14/14 21:37 .209 0017 08/14/14 21:40 .202 0018 08/15/14 09:45 .104</p> <p>Push No. 3 to erase, or power down to retain</p>														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#16

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008888
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP. (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014			14F23-11-5-10	.100	21		.101		X		Lee	17046	
			C1307252										
			Prepared by:										
			Douglas C. Talbot										
			06-23-14										
			Expires on:										
			06-23-16										

08/15/14 09:39
AS4 Serial no: 0000000
Version no: 4797

No. Date Time ZMAC
Calibration
08/25/13 10:45 .100

Test Result

0001	08/01/14	02:26	.142
0002	08/01/14	02:29	.139
0003	08/02/14	23:34	.154
0004	08/02/14	23:37	.149
0005	08/03/14	02:06	.132
0006	08/03/14	02:12	.129
0007	08/03/14	03:47	.148
0008	08/03/14	03:50	.101
0009	08/04/14	01:34	.207
0010	08/04/14	01:36	.201
0011	08/08/14	23:11	.126
0012	08/08/14	23:14	.129
0013	08/09/14	00:27	.000
0014	08/09/14	01:22	.170
0015	08/09/14	01:25	.119
0016	08/10/14	02:51	.154
0017	08/10/14	02:54	.164
0018	08/15/14	09:39	.101

Push Hd. 3 to erase,
or power down to retain

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#17

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008783
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP. (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	0940	34	14F23-11-5-10	.100	20						Lee	17046	
			C1307252										
Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16													

Test Result
 0001 08/06/14 02:16 .051
 0002 08/06/14 02:18 .048
 0003 08/07/14 23:47 .153
 0004 08/07/14 23:49 .155
 0005 08/15/14 09:53 .100
 No. Date Time ZHMC
 Calibration 07/18/08 13:52 .100
 08/15/14 09:53
 PAS Serial not 000783
 Version not 4/97
 Push No. 3 to erase
 or power down to return

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#19

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	LD. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008810
--------------------------------	-----------------	--------------------------------------	---------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP. (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	1000	34	14F23-11-5-10 C1307252	.100	20	.100			X		Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14</p> <p>Expires on: 06-23-16</p>													
<p>Test Result 0001 08/04/14 23:41 .074 0002 08/04/14 23:44 .076 0003 08/05/14 02:08 .609 0004 08/05/14 02:18 .664 0005 08/05/14 20:39 .168 0006 08/05/14 23:40 .164 0007 08/07/14 02:45 .062 0008 08/07/14 02:47 .066 0009 08/08/14 01:58 .000 0010 08/12/14 23:10 .132 0011 08/12/14 23:11 .144 0012 08/12/14 23:12 .137 0013 08/13/14 02:12 .159 0014 08/13/14 02:15 .160 0015 08/15/14 10:05 .100</p>													
<p>Push No. 3 to erase, or power down to retain</p>													
<p>08/15/14 10:05 No. Serial not 000810 Calibration not 4/97 18/38/03 09:53 .100</p>													

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#20

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018684
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1003	34	14F23-11-5-10	.100	22		.104			X		Lee	17046	
			C1307252											
			Prepared by: Douglas C. Talbot 06-23-14											
			Expires on: 06-23-16											
			<div style="border: 1px solid black; padding: 5px; width: fit-content;"> <p>08/15/14 10:06 NS4 Serial no: 018684 Version no: 4797</p> <p>No. Date Time %MC Calibration 11/03/11 16:03 .100</p> <p>Test Result 08/15/14 10:06 .104</p> <p>Push No. 3 to erase, or power down to retain</p> </div>											

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#21

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008635
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1005	34	14F23-11-5-10 C1307252	.100	21		.101			X		Lee	17046	
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											
<p style="text-align: center;"> Test Result 0001 08/05/14 23:59 .033 0002 08/06/14 00:01 .041 0003 08/06/14 01:44 .156 0004 08/06/14 01:47 .152 0005 08/13/14 01:20 .245 0006 08/13/14 01:23 .248 0007 08/15/14 10:11 .101 No. Date Time ZMNC Calibration 10/24/03 09:04 .100 08/15/14 10:11 AS4 Serial no: 600635 Version no: 4797 Push No. 3 to erase, or power down to retain </p>														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#22

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008845
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	1007	34	14F23-11-5-10 C1307252	.100	21		.104			X	Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16</p> <p style="text-align: center;"> No. Date Time ZMAC Calibration 12/24/03 11:01 .100 Test Result 0001 08/15/14 10:11 .104 Push No. 3 to erase. or power down to retain </p>													

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#23

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 082653
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1009	34	14F23-11-5-10 C1307252	.100	21		.101		X		Lee	17046		
<p>Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16</p>														
<p>Test Result 08/01/14 02:18 .006 08/01/14 02:20 .003 08/02/14 02:30 .002 08/02/14 02:39 .002 08/02/14 04:32 .004 08/02/14 04:35 .003 08/02/14 21:26 .150 08/02/14 21:29 .163 08/03/14 00:15 .065 08/04/14 01:50 .115 08/04/14 01:54 .156 08/09/14 02:49 .110 08/09/14 02:47 .107 08/09/14 06:00 .138 08/09/14 06:05 .134 08/10/14 00:17 .201 08/10/14 00:19 .170 08/10/14 00:22 .094 08/10/14 02:00 .186 08/10/14 02:05 .197 08/15/14 10:10 .101</p>														

Push No. 3 to erase
or power down to retain

08/15/14 10:11
AS4 Serial no: 082653
Version no: 4797
No. Date Time ZMAC
Calibration
02/17/14 10:08 100

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#24

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008848
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1011	34	14F23-11-5-10 C1307252	.100	20		.103			X		Lee	17046	
Prepared by: Douglas C. Talbot 06-23-14														
Expires on: 06-23-16														
<div style="border: 1px solid black; padding: 5px; display: inline-block;"> 08/15/14 10:17 NS4 Serial no: 0008948 Version no: 4792 No. Date Time 2000 Calibration 01/19/09 00:20 .100 Test Result 0001 08/15/14 10:16 .100 Push No. 3 to screen or power down to retain </div>														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#25

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 077591
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1014	34	14F23-11-5-10 C1307252	.100	20							Lee	17046	
			Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16											
			<div style="display: flex; justify-content: space-between;"> <div style="writing-mode: vertical-rl; transform: rotate(180deg);"> Test Result 0001 08/15/14 10:17 .101 Test No. 3 to erase. </div> <div style="writing-mode: vertical-rl; transform: rotate(180deg);"> Calibration 05/21/00 15:00 .100 No. Date Time ZONE </div> <div style="writing-mode: vertical-rl; transform: rotate(180deg);"> 08/15/14 10:18 NDA Serial no: 077591 Version no: 4797 </div> </div>											

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#26

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 009350
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	1015	34	14F23-11-5-10 C1307252	.100	21		.101			X	Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16</p>													
<p style="text-align: center;"> Test Result 08/15/14 10:24 .100 Calibration 08/02/06 09:00 .100 No. Date Time 2MAC Calibration 08/02/06 09:00 .100 Version no: 4297 08/15/14 10:24 AS4 Serial no: 000350 Version no: 4297 of power down to retain </p>													

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#27

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 077573
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	1020	34	14F23-11-5-10 C1307252	.100	21						Lee	17046	
Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16													
<div style="display: flex; justify-content: space-between;"> <div style="border: 1px solid black; padding: 5px;"> Push No. 3 to release or power down to retain </div> <div style="border: 1px solid black; padding: 5px;"> Test Result 08/01 08/03/14 19:56 .000 08/02 08/03/14 23:41 .054 08/03 08/04/14 01:03 .109 08/04 08/04/14 01:05 .112 08/05 08/04/14 21:04 .027 08/06 08/05/14 02:23 .163 08/07 08/05/14 02:26 .168 08/08 08/05/14 02:26 .021 08/09 08/12/14 00:19 .000 08/10 08/12/14 21:38 .131 08/11 08/12/14 21:41 .146 08/12 08/13/14 01:59 .097 08/13 08/13/14 02:00 .000 08/14 08/15/14 10:28 .006 </div> <div style="border: 1px solid black; padding: 5px;"> No. Date Time ZINC Calibration 04/09/14 00:36 .000 </div> <div style="border: 1px solid black; padding: 5px;"> 08/15/14 10:21 PAS Serial no: 077573 Version no: 4797 </div> </div>													

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#28

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 083051
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1022	34	14F23-11-5-10 C1307252	.100	21		.099			X		Lee	17046	
			Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16											
			<div style="border: 1px solid black; padding: 5px; width: fit-content; margin: auto;"> <p style="text-align: center;">No. Date Time %BAC Calibration 08/25/13 14:00 .100</p> <p style="text-align: center;">Test Result 0001 08/15/14 10:23 .099</p> <p style="text-align: center;">Push No. 3 to crases or power down to return</p> </div>											

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#30

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008897
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	1024	34	14F23-11-5-10 C1307252	.100	20	.107			X		Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16</p>													
<p>Test Result 0001 08/01/14 01:04 .795 0002 08/01/14 01:09 .174 0003 08/01/14 01:09 .193 0004 08/02/14 03:16 .167 0005 08/02/14 03:19 .167 0006 08/02/14 03:26 .183 0007 08/02/14 21:28 .156 0008 08/02/14 21:22 .161 0009 08/03/14 01:24 .260 0010 08/03/14 01:28 .253 0011 08/03/14 01:36 .163 0012 08/03/14 03:39 .154 0013 08/10/14 26:04 .666 0014 08/11/14 00:17 .078 0015 08/11/14 00:19 .081 0016 08/15/14 18:31 .107</p> <p>Push No. 3 to enter or power down to retain</p> <p>Mo. Date Time ZBAC Calibration 01/18/12 16:13 .100</p> <p>08/15/14 10:31 NSA Serial no: 000897 Version no: 4797</p>													

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#31

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018624
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS	
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES					NO
08/15/2014	10:27	34	14F23-11-5-10	.100	22		.098				X	Lee	17046	
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											
Test Result 0901 08/01/14 02:26 .071 0902 08/02/14 06:10 .078 0903 08/02/14 04:30 .140 0904 08/02/14 04:38 .140 0905 08/02/14 20:52 .132 0906 08/02/14 20:05 .132 0907 08/02/14 06:25 .102 0908 08/02/14 04:28 .096 0909 08/09/14 01:37 .131 0910 08/05/14 01:39 .129 0911 08/10/14 02:07 .050 0917 08/15/14 10:30 .098														
No. Date Time 200C Calibration 10/02/08 09:19 .100														
08/15/14 10:30 HSA Serial not 018624 Version not 4797														
Push No. 3 to erase, or Power down to Retain														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#32

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018646
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1031	34	14F23-11-5-10	.100	21		.099			X		Lee	17046	
			C1307252											
			Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16											
			<div style="border: 1px solid black; padding: 5px; width: fit-content; margin: auto;"> <p style="text-align: center;">No. Date Time %RMC Calibration 07/29/13 13:32 .100</p> <p style="text-align: center;">Test Result 0001 08/07/14 28:06 .117 0002 08/07/14 28:09 .128 0003 08/15/14 10:36 .099</p> <p style="text-align: center;">Push No. 3 to erase or power down to reload</p> </div>											

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#33

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 0774
--------------------------------	-----------------	--------------------------------------	----------------------	--	------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	1037	34	14F23-11-5-10	.100	21						Lee	17046	
			C1307252										
			Prepared by:										
			Douglas C. Talbot										
			06-23-14										
			Expires on:										
			06-23-16										

08/15/14 10:30
 004 SERIAL NO: 077400
 VERSION NO: 4709
 No. Date Time MMC
 Calibration
 05/21/08 14:35 .106
 Test Result
 000 08/15/14 10:30 .101
 Push No. 3 to erase,
 or power down to retain

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#34

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008877
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)*		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	1040	34	14F23-11-5-10 C1307252	.100	21		104			X	Lee	17046	

Prepared by:
Douglas C. Talbot
06-23-14
Expires on:
06-23-16

08/15/14 10:46
ASA Serial no: 008877
Version no: 4797
No. Date Time ZHNC
Calibration
05/26/08 10:40 100
Test Result
0001 08/15/14 10:46 104
Push No. 3 to reset
or power down to retain

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#36

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018015
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	1042	34	14F23-11-5-10	.100	22		099			X	Lee	17046	
			C1307252										
			Prepared by:										
			Douglas C. Talbot										
			06-23-14										
			Expires on:										
			06-23-16										

Test Result
 08/15/14 10:45 .099
 Calibration
 12/19/08 14:44 .100
 No. Date Time ZBNC
 08/15/14 10:45 018015
 Deviation no: 4797
 Push No. 3 to increase
 or power down for retain

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#37

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	LD. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018626
--------------------------------	-----------------	--------------------------------------	---------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP. (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	LD. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1044	34	14F23-11-5-10	.100	22		100				X	Lee	17046	
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

08/15/14 10:46
 AS4 Serial no: 018626
 Version no: 4797
 No. Date Time ZMNC
 Calibration 04/29/09 00:59 .100
 Test Result
 0001 08/15/14 10:46 .100
 Push No. 3 to screen,
 of power down to retain

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#38

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018696
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1103	34	14F23-11-5-10	.100	21		.107			X		Lee	17046	
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Test Result
 08/15/14 11:04 .107
 Calibration
 09/09/13 14:58 .100
 No. Date Time ZHMC
 08/15/14 11:05
 084 Serial no: 018696
 Version no: 4797
 Push No. 3 to erase
 or power down to retain

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#39

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 083030
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1105	34	14F23-11-5-10 C1307252	.100	21	.100			X		Lee	17046		
			Prepared by:	Douglas C. Talbot	06-23-14	Expires on:	06-23-16							
<p style="text-align: center;">No. Date Time /MNC Calibration 01/29/09 10:39 .100 Test Result 0001 08/15/14 11:06 .100 Push No. 9 to erase, or power down to retain</p>														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#3-40
 018692

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018692
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1 (Optional)	TEST #2 (Optional)	YES				
08/15/2014	1107	39	14F23-11-5-10 C1307252	.100	22	090			X		Lee	17046	
Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16													
Test Result 0001 08/15/14 11:11 .090 Calibration 08/12/08 14:35 .100 No. Date Time ZMAC 08/15/14 11:11 Serial No: 018692 Version No: 4797 Push No. 3 to erase or power down to retain													

* If the reading is within plus or minus (\pm) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#42

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018762
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1115	34	14F23-11-5-10	.100	21		.101				X	Lee	17046	
			C1307252											

Prepared by:
Douglas C. Talbot
06-23-14
Expires on:
06-23-16

Push No. 3 to erase,
or Power down to retain

Test Result
0801 08/15/14 11:18 .101

No. Date Time
Calibration
09/30/09 15:52 .100

08/15/14 11:18
NS4 Serial no: M10702
Version 001 4792

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

43

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018766
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	1118	34	14F23-11-5-10 C1307252	.100	22		.097			X	Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16</p> <p style="text-align: right;"> Test Result 08/01/14 03:02 .093 08/01/14 03:04 .093 08/02/14 04:19 .099 08/02/14 04:21 .099 08/03/14 05:14 .145 08/03/14 05:17 .147 08/15/14 00:26 .146 08/15/14 00:36 .160 08/15/14 00:32 .143 08/15/14 06:59 .105 08/15/14 02:08 .094 08/15/14 11:28 .097 </p> <p style="text-align: center;"> No. Date Time 2000 Calibration 08/12/12 12:36 100 </p> <p style="text-align: right;"> 08/15/14 11:21 654 Serial no: 010706 Version no: 4797 </p> <p style="text-align: center;"> Push Hdr. 3 to erase or power down to retain </p>													

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#44

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018691
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1121	34	14F23-11-5-10	.100	22		.102			X		Lee	17046	
			C1307252											
<p>Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16</p>														
<pre> 08/15/14 11:26 AS4 Serial not 018691 Version not 4797 No. Date Time ZMNC Calibration 09/08/08 14:01 .100 Test Result 0001 08/08/14 21:07 .000 0002 08/09/14 01:00 .100 0003 08/09/14 01:06 .114 0004 08/15/14 11:20 .100 Push Kn. 3 to erase or power down to retain </pre>														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#45

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 017990
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1123	34	14F23-11-5-10	.100	22	.10				X		Lee	17046	
			C1307252											
Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16														
<div style="float: right; border: 1px solid black; padding: 5px; text-align: right;"> 08/15/14 11:26 HSI Serial no: 017990 Version: not 4797 </div> <div style="float: right; border: 1px solid black; padding: 5px; text-align: right;"> No. Date Time ZONE Calibration 11/26/08 11:10 .100 </div> <div style="float: left; border: 1px solid black; padding: 5px;"> Test Result 0001 08/01/14 08:49 .049 0002 08/01/14 08:50 .049 0003 08/01/14 01:59 .000 0004 08/01/14 02:24 .000 0005 08/01/14 02:59 .172 0006 08/01/14 03:01 .175 0007 08/01/14 7:24 .038 0008 08/02/14 03:10 .038 0009 08/02/14 03:13 .037 0010 08/02/14 20:49 .196 0011 08/02/14 20:51 .210 0012 08/02/14 20:53 .200 0013 08/03/14 03:02 .214 0014 08/03/14 03:05 .219 0015 08/04/14 01:52 .000 0016 08/04/14 02:32 .014 0017 08/09/14 02:07 .037 0018 08/10/14 02:33 .102 0019 08/10/14 02:37 .140 0020 08/10/14 02:40 .134 0021 08/10/14 05:26 .153 0022 08/10/14 05:30 .138 0023 08/11/14 01:19 .032 0024 08/11/14 01:25 .060 0025 08/11/14 01:27 .061 0026 08/14/14 02:00 .030 0027 08/14/14 02:10 .030 0028 08/14/14 21:26 .049 0029 08/15/14 11:26 .106 </div> <div style="clear: both;"></div>														

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018774
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	1125	34	14F23-11-5-10 C1307252	.100	21	.101			X		Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14</p> <p>Expires on: 06-23-16</p>													
<p>Test Result 08/01 08/05/14 08:42 .041 08/02 08/05/14 08:44 .045 08/03 08/06/14 02:01 .139 08/04 08/06/14 02:05 .170 08/05 08/11/14 21:14 .177 08/06 08/11/14 21:17 .140 08/07 08/15/14 11:28 .101</p> <p>Push No. 5 to erase, or power down to retain</p> <p>Calibration 01/13/09 10:25 .100</p> <p>No. Date Time ZMAC 08/15/14 11:29 ASA Serial no: 018774 Version no: 4797</p>													

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#50

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 041486
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1127	34	14F23-11-5-10 C1307252	.100	21		.107			X		Lee	17046	
			Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16											
			Test Result 0001 08/15/14 11:31 .107 Calibration 09/08/06 10:56 .108 Ho. Date Time 2100 Version 04/99 08/15/14 11:31 004 serial no: 041486 001 4797											
			Push No. 3 to erase or power down to retain											

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#51

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 041495
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	113234		14F23-11-5-10	.100	20	.100			X		Lee	17046	
			C1307252										
Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16													
<div style="float: right; border: 1px solid black; padding: 5px; transform: rotate(180deg);"> 08/15/14 11:32 064 Serial not 041495 Version not 4797 No. Date Time 2000 Calibration 02/26/14 11:28 .100 Test Result 0001 08/15/14 11:32 .100 Push No. 3 to press or power down to retain </div>													

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051


#52

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 041502
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**			PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1134	34	14F23-11-5-10 C1307252	.100	21		.096		X		Lee	17046		
Prepared by: Douglas C. Talbot 06-23-14														
Expires on: 06-23-16														

Push No. 3 to erase, or power down to refresh.

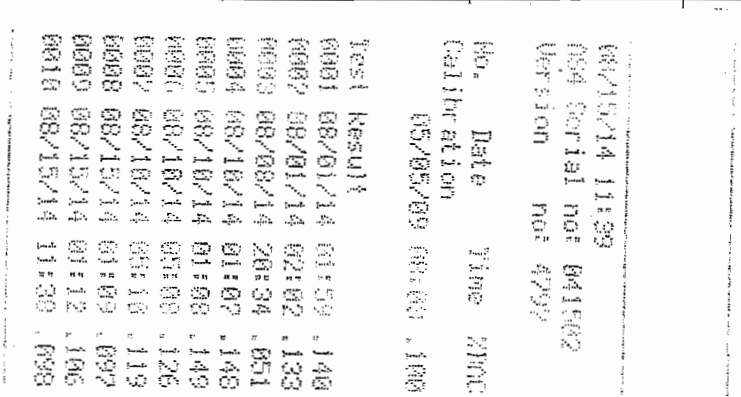

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#53

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 002654
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**			PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
08/15/2014	1137	34	14F23-11-5-10	.100	22		.099			X		Lee	17046	
			C1307252											

Prepared by:
Douglas C. Talbot
06-23-14
Expires on:
06-23-16

08/15/14 11:39
Test Serial No: 082654
Version No: 4797
No. Date Time ZMAC
Calibration
08/28/14 11:36 .100
Test Result
0801 08/15/14 11:39 .099
Push No. 3 to erase
or power down to retain

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

567

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008874
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)	PAS ACCURACY CHECK RESULTS*				CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.		VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014	1139	34	14F23-11-5-10 C1307252	.100	22		101			X		Lee	17046	
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

08/15/14 11:43
NSI Serial Num 008874
Version num 4797

No. Date Time Y/M/C
Calibration 08/28/14 11:48 .100

Test Result
0001 08/04/14 17:03 .110
0007 08/04/14 17:06 .111
0008 08/15/14 11:42 .101

Push Hp. 3 to clear
or Power down to reload

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#18

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO.
--------------------------------	-----------------	--------------------------------------	----------------------	--	----------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP. (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
08/15/2014			14F23-11-5-10	.100							Lee	17046	
			C1307252										NOT IN LOWER
			Prepared by:										
			Douglas C. Talbot										
			06-23-14										
			Expires on:										
			06-23-16										

* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).
 ** If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.