

S67.

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008874
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1505	34	14F23-11-5-10 C1307252	.100	22	.099			X		Lee	17046		
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Lost Result  
 Serial No. 10/23/2014 15:00:00  
 Calibration  
 No. Date Time Temp  
 06/20/14 11:40:00  
 Version Not OK/97  
 10/23/14 15:10  
 NS4 Serial No. 008874  
 Version Not OK/97  
 Turn down to retain

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

# 1

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 003501
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS												
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES					NO											
10/23/2014	0900	34	14F23-11-5-10 C1307252	.100	21		.096			X	Lee	17046													
<p>Prepared by: Douglas C. Talbot 06-23-14</p> <p>Expires on: 06-23-16</p> <p>Test Result</p> <table border="1"> <tr><td>0001</td><td>10/21/14</td><td>02:46</td><td>.114</td></tr> <tr><td>0002</td><td>10/21/14</td><td>02:48</td><td>.112</td></tr> <tr><td>0003</td><td>10/23/14</td><td>09:06</td><td>.096</td></tr> </table> <p>No. Date Time 2010 Calibration 09/08/09 15:40 .100</p> <p>Push No. 3 to erase, or power drain to retain</p> <p>10/23/14 09:07 AS4 Serial no: 000501 Version no: 4797</p>														0001	10/21/14	02:46	.114	0002	10/21/14	02:48	.112	0003	10/23/14	09:06	.096
0001	10/21/14	02:46	.114																						
0002	10/21/14	02:48	.112																						
0003	10/23/14	09:06	.096																						

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#2

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018785
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP. (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	0903	34	14F23-11-5-10 C1307252	.100	21		.099				X	Lee	17046	
			Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16											

Test Result  
0001 10/23/14 09:08 .099

Calibration  
07/16/08 10:22 .100

No. Date Time 2000  
Calibration

10/23/14 09:08  
AS4 Serial no: 018785  
Version no: 4797

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#3

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008546
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014	0906	34	14F23-11-5-10 C1307252	.100	22		.101			X	Lee	17046	

Prepared by:  
Douglas C. Talbot  
06-23-14  
Expires on:  
06-23-16

10/23/14 09:10  
 AS4 Serial no: 008546  
 Version no: 4297  
 No. Date Time 2000:  
 Calibration 06/28/13 10:06 .100  
 Test Result  
 0001 10/19/14 21:42 .021  
 0002 10/23/14 09:10 .101  
 Push No. 3 to erase,  
 or power down to retain

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#4

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 082659
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014	0909	34	14F23-11-5-10 C1307252	.100	21		.099			X	Lee	17046	
			Prepared by:										
			Douglas C. Talbot										
			06-23-14										
			Expires on:										
			06-23-16										

10/23/14 09:13  
 AS4 Serial no: 082659  
 Version no: 4797  
 No. Date Time 2000  
 Calibration 03/28/14 09:04 .100  
 Test Result  
 0001 10/23/14 09:12 .099  
 Push No. 3 to erase,  
 or power down to retain

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#5

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 003559
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)	PAS ACCURACY CHECK RESULTS*				CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	ID. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.		VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014			14F23-11-5-10	.100								Lee	17046	OUT for Service
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#6

AREA NAME	AREA NO.	COORDINATOR NAME	I.D. NUMBER	PAS MAKE/MODEL	PAS SERIAL NO.
South Los Angeles	530	Officer Kirk Lee	17046	Intoximeters Inc./Alco-Sensor IV	008580

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	ID NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	0911	34	14F23-11-5-10	.100	21		.099				X	Lee	17046	
			C1307252											

Prepared by:  
Douglas C. Talbot  
06-23-14  
Expires on:  
06-23-16

Test Result  
 0.099 10/22/14 09:17  
 0.100 10/22/14 09:16  
 0.100 10/22/14 09:15  
 No. Date Time ZONE  
 Calibration 08/06/14 12:30 1000  
 10/23/14 09:17  
 AS4 Serial no: 008580  
 Version no: 4/97

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#7

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 093032
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014	0913	34	14F23-11-5-10	.100	21		.100			X	Lee	17046	
			C1307252										
			Prepared by:										
			Douglas C. Talbot										
			06-23-14										
			Expires on:										
			06-23-16										
													Test Result 0001 10/21/14 22:50 .010 0002 10/21/14 22:52 .010 0003 10/23/14 09:12 .100 No. Date Time 2000 Calibration 02/17/14 09:01 .100 10/23/14 09:13 AS4 Serial no: 003002 Version no: 4797
													Push No. 3 to erase, or power down to retain

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.



# PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#3

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008620
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**			PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	0915	34	14F23-11-5-10 C1307252	.100	21		.099			X		Lee	17046	
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

10/23/14 09:48  
AS4 Serial not (808)20  
Version not 4797

No. Date Time XMP  
Calibration  
01/28/13 14:34 .100

Test Result  
0901 10/21/14 03:55 .169  
0902 10/21/14 03:57 .172  
0903 10/23/14 09:25 .099

Push No. 3 to erase,  
or power down to retain

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#9

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 082957
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	0930	34	14F23-11-5-10	.100	22		.099			X		Lee	17046	
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Push No. 3 to erase,  
or power down to retain

Test Result  
0001 10/23/14 09:42 .100

No. Date Time %NAC  
Calibration  
02/17/14 09:52 .100

10/23/14 09:43  
MS4 Serial not received  
Version not 4/97

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#10

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 077505
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014	0933	34	14F23-11-5-10 C1307252	.100	21		.099			X	Lee	17046	
			Prepared by:										
			Douglas C. Talbot										
			06-23-14										
			Expires on:										
			06-23-16										

10/23/14 09:43  
 884 Serial not W/PMS  
 Version not 4/97  
 No. Date Time ZMAC  
 Calibration 10/18/14 07:21 .099  
 Test Result  
 0001 10/23/14 09:42 .098  
 Push No. 3 to erase,  
 or power down to retain.

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

# 11

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 077479
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	0936	34	14F23-11-5-10 C1307252	.100	22		.097			X		Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16</p> <p>10/23/14 09:48 054 Serial no: 077479 Version: 001 4797</p> <p>No. Date Time %BAC Calibration 07/17/14 09:10 .100</p> <p>Test Result 001 10/23/14 09:47 .097</p> <p>Push No. 3 to erase, or power down to retain</p>														

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#12

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 082660
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**			PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	0939	34	14F23-11-5-10	.100	21		.099			X		Lee	17046	
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Push No. 3 to erase,  
or power down to retain.

10/23/14 09:50	NS4 Serial no: 082660	Version no: 4/07
No. Date Time ZBAC	Call#	ation
02/12/14 09:16 .100		
Test Result		
0001 10/17/14 22:58 .112		
0002 10/17/14 22:52 .106		
0003 10/18/14 08:31 .196		
0004 10/18/14 08:33 .195		
0005 10/23/14 09:50 .099		

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#13

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008709
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	0942	34	14F23-11-5-10 C1307252	.100	22		.101			X		Lee	17046	
			Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16											

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

#14

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008714
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	0945	34	14F23-11-5-10	.100	22		0.102		X		Lee	17046		
			C1307252											

Prepared by:  
Douglas C. Talbot  
06-23-14  
Expires on:  
06-23-16

19/7/2014 19:03  
AS4 Serial not 008714  
Version not 4797

No. Date Time XIMC  
Calibration 03/11/04 14:55 .100

Test Result  
0001 10/10/14 03:22 .207  
0002 10/10/14 03:24 .204  
0003 10/10/14 22:25 .100  
0004 10/10/14 22:27 .110  
0005 10/10/14 22:30 .122  
0006 10/19/14 08:45 .140  
0007 10/19/14 08:48 .132  
0008 10/19/14 23:46 .043  
0009 10/23/14 10:03 .102

Push Ho. 3 to erase,  
or power down to retain

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

# 16

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008338
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**			PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	0948	34	14F23-11-5-10 C1307252	.100	22		.099			X		Lee	17046	
Prepared by: Douglas C. Talbot 06-23-14														
Expires on: 06-23-16														
<p>Test Result</p> <p>0001 10/10/14 23:17 .152</p> <p>0002 10/10/14 23:19 .135</p> <p>0003 10/10/14 23:22 .147</p> <p>0004 10/10/14 02:04 .161</p> <p>0005 10/19/14 02:07 .159</p> <p>0006 10/23/14 09:54 .099</p>														
<p>Calibration</p> <p>06/25/10 10:45 .100</p>														
<p>Push No. 3 to erase or Power down to retain</p>														

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.



**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#17

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008783
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014	0951	34	14F23-11-5-10 C1307252	.100	20		.101			X	Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16</p>													
<p>Test Result 0001 10/28/14 22:54 .106 0002 10/28/14 22:56 .165 0003 10/28/14 02:16 .146 0004 10/28/14 02:19 .146 0005 10/28/14 10:07 .101</p> <p>No. Date Time XMNC Calibration 07/18/08 13:52 .100</p> <p>10/28/14 10:07 004 serial no: 000703 Version no: 4797</p> <p>Push No. 0 to erase or power down to retain</p>													

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#18

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 082657
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	0954	34	14F23-11-5-10 C1307252	.100	21							Lee	17046	
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Test Result  
 0001 10/23/14 10:00 .100  
 No. Date Time %MC  
 Calibration 02/17/14 09:50 .100  
 Version not 4797  
 10/23/14 10:00  
 AS4 Serial no: 082657  
 User: 100

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#19

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 009810
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1105	34	14F23-11-5-10	.100	21		.097			X		Lee	17046	
			C1307252											
			Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16											
			<div style="border: 1px solid black; padding: 5px; width: fit-content; margin: auto;"> <p style="text-align: center;">Push No. 3 to erase or power down to retain</p> <p style="text-align: center;">Test Result 0001 10/23/14 11:15 .097</p> <p style="text-align: center;">No. Date Time 2BAC Calibration 10/30/08 09:50 .100</p> <p style="text-align: center;">10/23/14 11:16 test serial no: 000810 version no: 4797</p> </div>											

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#20

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018684
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014	1108	34	14F23-11-5-10 C1307252	.100	22		.101			X	Lee	17046	

Prepared by:  
Douglas C. Talbot  
06-23-14  
Expires on:  
06-23-16

Fuel No. 9. Lo across  
of power down to refuel  
 Test Result  
0001 10/23/14 11:16 .100  
 No. Date Time %BAC  
Calibration  
11/03/11 16:00 .100  
 10/23/14 11:16  
 NS4 serial not 018684  
Version not 4797

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#21

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008635
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1111	34	14F23-11-5-10 C1307252	.100	21		.101			X		Lee	17046	
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Test Result  
 0001 10/21/14 01:47 .110  
 0002 10/21/14 01:51 .109  
 0003 10/21/14 01:48 .102  
 0004 10/20/14 11:20 .100

No. Date Time ZHMC  
 Calibration 10/24/03 09:04 .100

10/23/14 11:24  
 NS4 serial no: 008635  
 version no: 4797

Push No. 3 to zeroes  
 or power down for 1 min

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#22

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008845
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**			PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1114	34	14F23-11-5-10	.100	21		.102			X		Lee	17046	
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Push the 3 buttons  
or power down to regain  
 Test Result  
 0001 10/23/14 11:25 .100  
 No. Date Time ZINC  
 Calibration  
 12/24/09 11:01 .100  
 Version no: 4797  
 10/23/14 11:25  
 PC Serial no: 000845  
 Version no: 4797

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#23

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 082653
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)		PAS TEMP. (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1117	34	14F23-11-5-10 C1307252	.100	21		.099			X		Lee	17046	
			Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16											
			<div style="border: 1px solid black; padding: 5px; width: fit-content; margin: auto;"> <p style="text-align: center;">No. Date Time HMM</p> <p style="text-align: center;">Calibration</p> <p style="text-align: center;">02/17/14 10:00 100</p> <hr/> <p style="text-align: center;">Test Result</p> <p style="text-align: center;">0001 10/23/14 11:24 .099</p> <hr/> <p style="text-align: center;">Push Box 3 to screen of liquor down to replace</p> </div>											

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#24  
008848

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008848
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**			PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1120	34	14F23-11-5-10 C1307252	.100	21		.100			X		Lee	17046	
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Test Result  
 0001 10/22/14 07:06 .100  
 0002 10/23/14 11:35 .100  
 No. Date Time ZPMG  
 Calibration  
 01/13/03 00:25 .100  
 Version no: 4797  
 PAS Serial no: 008848  
 10/23/14 11:37

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.



**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#25

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 077591
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014	1123	34	14F23-11-5-10 C1307252	.100	20		.100			X	Lee	17046	
Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16													
Test Result 0001 10/23/14 11:40 100 Calibration 05/21/08 15:00 100 No. Date Time ZMPC Calibration 05/21/08 15:00 100 Version not 4797 10/23/14 11:41 PAS Serial not 077591 Version not 4797													

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#26

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008850
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	11:26	34	14F23-11-5-10 C1307252	.100	21		.101			X		Lee	17046	
			Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16											

Test Result  
 0001 10/21/14 11:04 PAS  
 0002 10/23/14 11:58 310  
 No. Date Time 2BAC  
 Calibration 09/02/06 09:07 .100  
 10/23/14 11:58  
 NS4 Control num: 0088050  
 Version 4797

or down to return

\* If the reading is within plus or minus ( $\pm$ ) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#27

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 077573
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**			PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1129	34	14F23-11-5-10 C1307252	.100	22		.095			X		Lee	17046	
Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16														
<p>Test Result</p> <p>0001 10/21/14 02:39 .218</p> <p>0002 10/21/14 02:39 .215</p> <p>0003 10/23/14 00:28 .104</p> <p>0004 10/23/14 00:28 .100</p> <p>0005 10/23/14 11:42 .100</p> <p>Push the 2 to check or power down to retain</p> <p>No. Date Time XIDAC Calibration 04/09/14 08:36 .804</p> <p>10/23/14 11:42 004 Serial no: 077573 Division no: 4797</p> <p>or power down to retain</p>														

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#28

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 083051
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014	1132	34	14F23-11-5-10 C1307252	.100	21	.099			X		Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14</p> <p>Expires on: 06-23-16</p>													
<p>Test Result 0001 06/23/14 11:46 .100</p> <p>Calibration 09/25/13 14:00 .100</p> <p>No. Date Time 2BAC Calibration 09/25/13 14:00 .100</p> <p>10/23/14 11:53 PAS serial no: 083051 Version not 4797</p>													

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#30

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 003897
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1136	34	14F23-11-5-10	.100	21							Lee	17046	
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Push No. 9 to erase  
or power down to retain

Test Result  
 0001 10/11/14 02:21 000  
 0002 10/11/14 02:24 100  
 0003 10/12/14 04:05 000  
 0004 10/12/14 00:05 100  
 0005 10/12/14 04:00 100  
 0006 10/12/14 04:00 100  
 0007 10/12/14 04:18 220  
 0008 10/12/14 04:12 201  
 0009 10/12/14 04:37 205  
 0010 10/12/14 04:39 214  
 0011 10/12/14 04:49 004  
 0012 10/12/14 04:51 004  
 0013 10/12/14 03:46 000  
 0014 10/12/14 03:48 000  
 0015 10/12/14 03:49 000  
 0016 10/12/14 03:50 100  
 0017 10/12/14 04:22 000  
 0018 10/12/14 04:28 000  
 0019 10/12/14 04:34 000  
 0020 10/12/14 04:35 000  
 0021 10/12/14 04:35 002  
 0022 10/12/14 04:36 210  
 0023 10/12/14 04:28 209  
 0024 10/20/14 04:55 025  
 0025 10/20/14 04:24 172  
 0026 10/20/14 02:22 176  
 0027 10/23/14 12:05 106

10/20/14 12:03  
 Not Serial not 000097  
 Version not 4797  
 No. Date Time ZHNC  
 Calibration  
 01/19/12 16:13 100

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#31

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 019624
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)*		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	12:00	34	14F23-11-5-10 C1307252	.100	22		.096			X		Lee	17046	
<p>Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16</p>														
<p style="text-align: center;">             10/23/14 12:17              AS4 SERIAL NO: 815224              Version: 10/09/08              No. Tests: Time: 2000              Calibration: 10/09/08 08:19 .100              Test Result: 800 10/23/14 12:22 .096              Push No. 3 to press              or power down to retain         </p>														

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

#32

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018646
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**			PAS TEMP. (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1203	30	14F23-11-5-10	.100	22		.099			X		Lee	17046	
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Push No. 8 to erase  
 or power down to retain  
 5-1 Result  
 0001 10/23/14 12:25 .099  
 07/29/13 13:32 .100  
 No. into time ZINC  
 calibration  
 10/23/14 12:03  
 PAS serial no. 018646  
 Dev. no. 900 4797

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

# 33

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 077438
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014	12:00	34	14F23-11-5-10 C1307252	.100	21		.101			X	Lee	17046	
<p>Prepared by: Douglas C. Talbot</p> <p>06-23-14</p> <p>Expires on: 06-23-16</p>													
<p>10/23/14 12:00 PAS Serial no 077438 Device no 1297 No. Tests Done 2000 Call ID 11001 06/23/09 14:35 .100</p> <p>Test result 0001 10/23/14 12:39 .101</p> <p>Push Ho. 9 to erase, or power down to retain</p>													

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).

\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.



**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#34

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 008877
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	12:09	34	14F23-11-5-10	.100	21		.102				X	Lee	17046	
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Test Result  
 10/23/14 12:09  
 10/23/14 12:49 .102  
 10/26/05 10:40 .100  
 Test No. 3 to erase,  
 or power down to retain

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#35

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018615
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)*		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1248	34	14F23-11-5-10	.100	23		.095				X	Lee	17046	
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Test Result  
 AM9 10/23/14 12:55 .095  
 Calibration  
 12/19/08 14:44 .100  
 NO. 1411 TIME 2005  
 10/23/14 12:55  
 PAS Serial No. 018615  
 Version 101 12/02

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

#37

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 019626
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1400	34	14F23-11-5-10	.100	22		.098			X		Lee	17046	
			C1307252											
			Prepared by:											
			Douglas C. Talbot											
			06-23-14											
			Expires on:											
			06-23-16											

Test No. 3 to erase  
 or power down to retain  
 Test Result  
 0001 10/23/14 14:15 .098  
 No. Make Time 23MC  
 Calibration  
 06/29/01 00:59 .101  
 10/23/14 14:15  
 654 00000 000 000000  
 00000 000 0000

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

#38

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018696
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**			PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1414	34	14F23-11-5-10 C1307252	.100	22		101			X		Lee	17046	
			Prepared by: Douglas C. Talbot 06-23-14											
			Expires on: 06-23-16											

Test Result  
001 10/23/14 14:23 .101  
SN/99/12 14150 100  
No. 1144 1100 2310  
02/12/13  
08/09/12 14150 100  
10/23/14 14:58  
684 Serial no: 610006  
Def: 101 100 8797

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

#39

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 083030
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014	1428	34	14F23-11-5-10	.100	22		.097			X	Lee	17046	
			C1307252										
			Prepared by:										
			Douglas C. Talbot										
			06-23-14										
			Expires on:										
			06-23-16										

Test Result  
 16/18/14 02:03 .103  
 16/18/14 02:07 .101  
 16/18/14 20:36 .058  
 16/18/14 20:31 .059  
 16/19/14 00:01 .113  
 16/19/14 00:04 .115  
 16/19/14 04:19 .175  
 16/19/14 04:21 .179  
 16/20/14 00:28 .073  
 16/20/14 00:22 .073  
 16/20/14 01:57 .140  
 16/21/14 02:00 .140  
 16/23/14 14:01 .097

Push No. 9 to erase  
 or power down to retain

or power down to retain

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

### PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG

CHP 202K (Rev. 8-08) OPI 051

#40

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018692
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1431	34	14F23-11-5-10 C1307252	.100	22		.099			X		Lee	17046	
<div style="display: flex; justify-content: space-between; align-items: flex-start;"> <div style="width: 30%;"> <p>Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16</p> </div> <div style="width: 60%; border: 1px solid black; padding: 5px;"> <p style="text-align: center;">test result 10/23/2014 14:32 099 No. 11416 Calibrated on 10/12/2014 14:26 100</p> </div> </div>														

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.



**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#43

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018766
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014			14F23-11-5-10	.100								Lee	17046	Out for service
			C1307252											

Prepared by:  
 Douglas C. Talbot  
 06-23-14  
 Expires on:  
 06-23-16

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.



**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051


#44

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018691
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1437	34	14F23-11-5-10	.100	22		.100		X		Lee	17046	
			C1307252										

Prepared by:  
Douglas C. Talbot  
06-23-14  
Expires on:  
06-23-16

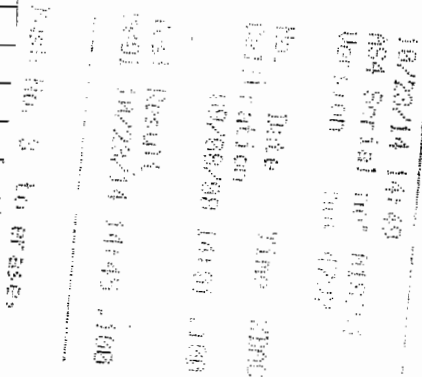

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#45

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 017990
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1447	34	14F23-11-5-10	.100	22		.106			X		Lee	17046	
			C1307252											
Prepared by: Douglas C. Talbot 06-23-14 Expires on: 06-23-16														

Push the 2 to erase  
or power down to refresh

Test Results  
10/21/14 20:30 100  
10/21/14 20:39 100  
10/22/14 01:47 106  
10/22/14 21:40 187  
10/23/14 14:56 166

No. Date Time %MC  
Calibration  
11/26/09 11:18 100

10/23/14 14:54  
854 Serial no: 147990  
Version no: 4797

or power down to refresh

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#46

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 018774
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1 (Optional)	TEST #2 (Optional)	YES				
10/23/2014	1453	34	14F23-11-5-10	.100	21		.099			X	Lee	17046	
			C1307252										
			Prepared by:										
			Douglas C. Talbot										
			06-23-14										
			Expires on:										
			06-23-16										

Test Result:  
 10/23/14 14:53  
 001 10/21/14 20:49 .079  
 002 10/21/14 20:52 .006  
 003 10/23/14 14:58 .099  
 Test No. 3 to 0900  
 or power down to retain  
 10/23/09 10:20 .100  
 Date Time 2010  
 10/23/09 10:20 .100  
 10/23/09 10:20 .100

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

#50

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 041486
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES				
10/23/2014	1450	34	14F23-11-5-10	.100							Lee	17046	out for service
			C1307252										
			Prepared by:										
			Douglas C. Talbot										
			06-23-14										
			Expires on:										
			06-23-16										

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

**PRELIMINARY ALCOHOL SCREENING (PAS) DEVICE ACCURACY CHECK/CALIBRATION LOG**

CHP 202K (Rev. 8-08) OPI 051

#51

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 041495
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1456	34	14F23-11-5-10 C1307252	.100	21		.100			X		Lee	17046	

Prepared by:  
Douglas C. Talbot  
06-23-14  
Expires on:  
06-23-16

No. 1446 Jim Bink  
 Calibration  
 06/26/14 11:28 AM  
 Test Result  
 0.1028/14 14:56 100  
 Push Ho. 2 to turn on  
 or power down to piston

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

#52

AREA NAME South Los Angeles	AREA NO. 530	COORDINATOR NAME Officer Kirk Lee	I.D. NUMBER 17046	PAS MAKE/MODEL Intoximeters Inc./Alco-Sensor IV	PAS SERIAL NO. 041502
--------------------------------	-----------------	--------------------------------------	----------------------	--	--------------------------

**PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.**

DATE	TIME	TEMP (°C)	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/ COMMENTS
			LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES	NO				
10/23/2014	1459	34	14F23-11-5-10 C1307252	.100	21		.098			X		Lee	17046	

Prepared by:  
Douglas C. Talbot  
06-23-14  
Expires on:  
06-23-16

Test Result  
0400 10/18/14 04:16 .148  
0407 10/18/14 04:19 .147  
0408 10/18/14 20:54 .119  
0404 10/18/14 20:57 .121  
0405 10/23/14 10:00 .098

Push 10, 5 to review  
of history down to bottom

10/23/14 11:00  
10/23/14 10:00  
10/23/14 09:00  
10/23/14 08:00

10/23/14 08:00  
10/23/14 07:00  
10/23/14 06:00  
10/23/14 05:00  
10/23/14 04:00

10/23/14 03:00  
10/23/14 02:00  
10/23/14 01:00  
10/23/14 00:00

10/23/14 00:00  
10/23/14 00:00  
10/23/14 00:00  
10/23/14 00:00

\* If the reading is within plus or minus (±) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
\*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.

#53

AREA NAME	AREA NO.	COORDINATOR NAME	I.D. NUMBER	PAS MAKE/MODEL	PAS SERIAL NO.
South Los Angeles	530	Officer Kirk Lee	17046	Intoximeters Inc./Alco-Sensor IV	082654

PAS DEVICES SHALL BE CHECKED FOR ACCURACY EVERY 10 DAYS OR EVERY 150 TESTS, WHICHEVER OCCURS FIRST.

DATE	TIME	SIMULATOR SOLUTION (OR DRY GAS)**		PAS TEMP (°C)		PAS ACCURACY CHECK RESULTS*		CALIBRATION REQUIRED		PAS RETEST RESULTS	OPERATOR	I.D. NO.	REPAIRS/PROBLEMS/COMMENTS	
		TEMP (°C)	LOT NO.	VALUE	TEST #1	TEST #2 (Optional)	TEST #1	TEST #2 (Optional)	YES					NO
10/23/2014	1502.34		14F23-11-5-10	.100	22		.100				X	Lee	17046	
			C1307252											

Prepared by:  
 Douglas C. Talbot  
 06-23-14  
 Expires on:  
 06-23-16

Test Result

06/16/2014	06/23/14	.100
06/17/2014	06/23/14	.100
06/18/2014	06/23/14	.100
06/19/2014	06/23/14	.100
06/20/2014	06/23/14	.100
06/21/2014	06/23/14	.100
06/22/2014	06/23/14	.100
06/23/2014	06/23/14	.100
06/24/2014	06/23/14	.100
06/25/2014	06/23/14	.100
06/26/2014	06/23/14	.100
06/27/2014	06/23/14	.100
06/28/2014	06/23/14	.100
06/29/2014	06/23/14	.100
06/30/2014	06/23/14	.100

\* If the reading is within plus or minus ( $\pm$ ) 0.010 percent of the actual value of the alcohol solution, no calibration is required (e.g., with a 0.100 percent solution, an acceptable range is 0.090 to 0.110).  
 \*\* If using dry gas for accuracy checks, note the canister serial number in the lot no. column. If needed, calibration shall be performed with a wet bath simulator.